BIOBOON BIOTECH LLC



H. PYLORI Ag Rapid Test Kit (Stool)

Detect H. Pylori for a Healthier Tomorrow

Rapid | Reliable | Accurate

A rapid chromatographic immunoassay for the qualitative detection of Helicobacter pylori Antigen in human stool specimens.

- High Accuracy
- Rapid Results (15–20 Minutes)
- Do not Interpret Results After 30 Minutes.
- Stool Test
- For In Vitro Diagnostic Use Only



INTERPRETATION OF RESULTS

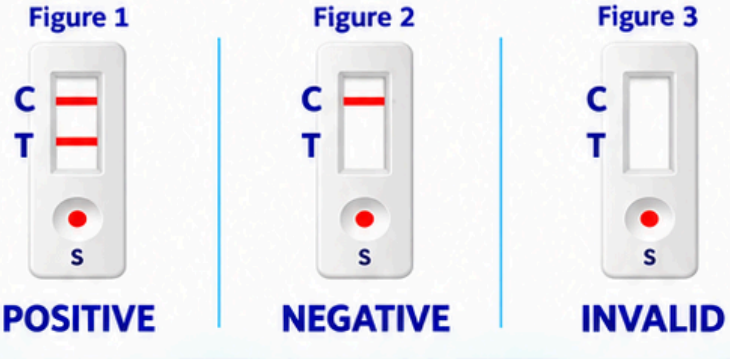



DIRECTIONS FOR USE

1. Allow test device, Assay Buffer and specimen equilibrates to room temperature (15–30 °C) prior to testing.
2. Remove the test device from the aluminum foil pouch and use it as soon as possible. Best results will be obtained if the assay is performed within one hour.
3. Unscrew the cap of the specimen collection tube with extraction buffer, then randomly stab the specimen collection applicator into the fecal specimen at least 3 different sites. Take the dab of stool sample using applicator and add it to the 1 mL buffer in sample extraction tube. Mix well then kept for 10 minute.
   Add 2 drops (80 to 100 µL) into the sample well.
4. Allow reaction to occur and read the results at 20 minutes. Do not interpret results after 30 minutes.

India Office
BIOBOON BIOTECH INDIA LLP
207. Regent Square
2nd floor, Above D'mart shopping mall
Adajan, Surat-395009
Email : info@bioboonbiotech.com

USA Address:-
BIOBOON BIOTECH LLC
1526 West 3rd Street,
Plainfield, NJ, 07063, USA
Email : mahipal@bioboonbiotech.com