BIOBOON BIOTECH LLC

HCG – Pregnancy Rapid Test Strip

(DIP STICK)



Read results at **3 minutes** for urine



INTERPRETATION OF RESULTS

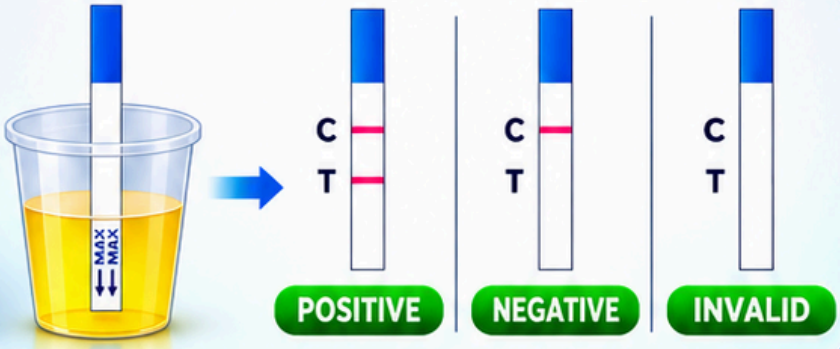

DIRECTIONS FOR USE

1. Allow test strip and urine sample to reach room temperature (20–30°C).
2. Remove the test strip from the foil pouch and use immediately within one hour.
3. Immerse the absorbent tip at least two-thirds in urine in a clean cup for at least 20 seconds.
4. Lay the test strip on a clean and stable surface, and start the timer immediately.

INTERPRETATION OF RESULTS

Negative:	Only one pink line appears in the Control area.
Positive:	A distinguishable pink-rotse colored line also appears in the Test region in addition to the Control line, indicating HCG in the sample.
Invalid:	If no line appears in control and test regions, or if only test line appears without control line, repeat with a fresh strip.

PERFORMANCE

- Relative Sensitivity: >99.9% (98.7%–100%)
- Relative Specificity: >99.9% (99.2%–100%)
- Overall Accuracy: >99.9% (99.5%–100%)
- 95% confidence intervals

COMPARISON RESULTS

Method	HCG Rapid Test		Comparator		Total Samples
	Positive	Negative	Positive	Negative	
Results	163	280	163	280	543

No discordant results
(163 positive matches, 280 negative matches).

INDIA OFFICE
BIOBOON BIOTECH INDIA LLP
207. Regent Square
2nd floor, Above D'mart shopping mall
Adajan
Surat-395009
Email: info@bioboonbiotech.com

USA ADDRESS
BIOBOON BIOTECH LLC
1526 West 3rd Street,
Plainfield, NJ, 07063
USA
Email: mahipal@bioboonbiotech.com